

Original Article

Comparison of Serum Stability Against Uric Acid and Glucose

Nur Vita Purwaningsih¹, Ellies Tunjung Sari Maulidyanti^{1*}, Rahma Widyastuti¹

¹Department of Medical Laboratory Technology, Faculty of Health Sciences,
Muhammadiyah University of Surabaya, Surabaya 60113, Indonesia

*Corresponding Author:

Ellies Tunjung Sari Maulidyanti, Bach.AppSc, M.Sc

Department of Medical Laboratory Technology, Faculty of Health Sciences, Muhammadiyah
University of Surabaya, 60113, Indonesia

Sutorejo Street No. 59 Surabaya 60113, East Java, Indonesia

Tel.: 085857535551

Email: elliestunjungismail@gmail.com

ABSTRACT

The selection of tools, especially the use of vacutainer tubes, affects the results of the examination to determine the stability of serum from plain vacutainer with vacutainer separation gel on the quality of uric acid and glucose test results. This study used an experimental design. The study took blood samples of 3 ml each in SST vacutainer and plain vacutainer serum. The mean uric acid levels using plain vacutainer and SST vacutainer were 4.5875 ± 0.59048 and 4.9250 ± 0.56318 , respectively. The mean glucose levels using plain vacutainer and SST vacutainer were 90.64 ± 12.33 and 94.12 ± 13.30 , respectively. Uric acid and glucose levels using gel-separated vacutainer were higher than uric acid levels using plain vacutainer. There was a significant difference in uric acid levels between regular vacutainers and SST vacutainers, similar to glucose levels ($p = 0.000$, $p = 0.000$). Uric acid and glucose levels using SST vacutainer were higher than uric acid levels using plain vacutainer. The following types of vacutainer separator gel and plain vacutainer affect the quality of uric acid and glucose test results.

KEYWORDS: Uric Acid Levels, Glucose levels, Pre-Analytics, Serum, Vacutainer Separator Gel, Vacutainer

INTRODUCTION

Good laboratory practice is an essential part of good manufacturing practice. It involves a number of good practices in the quality control (QC) laboratory which are to be undertaken to carry out an analysis with a defined degree of accuracy and precision¹. Clinical laboratories are an integral part of health services. For example, specimen examination, laboratory service errors and errors that arise during the service can be detrimental to the patient². The pre-analytic stage uses 61%, 25% analytical stage, and 14% post-analytic of the total error³. Maintaining the stability of blood analytes during sample storage is a significant issue in clinical laboratories. Typically, samples are stored in the refrigerator's door (4–8°C) for a brief amount of time or in the freezer (-20°C) for an extended period of time⁴. Numerous methods for improving the quality of pre-analytic and analytic⁵, besides that laboratory performance can be determined by evaluated the human errors analysis of materials or specimens⁶.

Accurate laboratory testing necessitates an understanding of the interactions between the collection tube and the blood specimen, which can affect the reliability of laboratory test results. However, due to the frequent occurrence of examination delays, blood specimen examinations shall be conducted immediately following the collection of samples⁷⁻⁹. One of the tools that must exist in the pre-analytic process is a blood collection tube (vacutainer) are used for serum collection for specific chemical tests, and serum gel tubes containing clot

activators and gel separators are used for various laboratory tests¹⁰. Collecting samples, transporting them, and centrifuging them are also critical steps in the laboratory process. Serum Separator Tubes (SST) are observed during centrifugation, along with a gel barrier that has moved to the serum/clot interface¹¹.

Centrifugation at low speed for a brief period of time to obtain plasma or serum may result in insufficient separation of cellular blood components, while prolonged centrifugation at high speed may result in hemolysis and cell damage. The use of serum is preferred in clinical examination over plasma because does not use additional anticoagulants, the components contained in the serum are not disturbed in terms of activity and reaction to the results¹². Prior to processing the sample, stability limits for each analyte and sample used as the basis for rejection must be determined⁵. The stability limit of an analyte is defined as the time point at which the analyte's percent deviation (PD%) reaches the maximum permissible error. Although many experimental studies have been conducted to determine the stability of most laboratory analytes under various conditions, there are some clinical guidelines that include general laboratory recommendations¹³.

Blood collection tubes have a number of limitations, including an inability to store blood samples for an extended period of time and difficulty separating ~~blood~~ serum from red blood cells¹⁴. Additionally, prolonged contact between serum and blood cells can cause lysis. To address this issue, a SST was introduced that contained silica and polymer gel for serum separation. At the tube's end, the serum separator gel acts as a stable chemical and physical barrier between serum and clotted blood. The ~~blood~~ serum separating gel significantly increases the stability of the serum, providing convenience in storage and transport^{15,16}. The most critical factors affecting the serum separator gel's position in the SST tube are viscosity and density, centrifugation speed, temperature, and storage conditions. However, commercially available separation gels are expensive and have several performance limitations, including instability for certain analytes, polymer gels under extreme temperature conditions, the presence of gel parts or oily layers in serum, and absorption of certain substances and some steroid hormones into the gel¹⁷.

Vacutainer plain is a tube that does not contain anticoagulants so that the test material is not contaminated and can affect the examination, so that the blood can clot naturally. According to the National Committee Clinical Laboratory System, the ideal clotting time is about 60 minutes. The advantage of vacutainers plain are relatively cheap and easy to obtain¹⁸. SST tubes contain silica particles and serum separation gel, frozen for approximately 15-30 minutes, freeze relatively quickly and produce higher serum levels¹⁹.

Blood glucose examination is very important in clinical laboratories, especially diabetic patients to control carbohydrate intake in eating tests and oral glucose tolerance tests^{20,21}. Diabetes mellitus is a metabolic disorder syndrome characterized by high blood glucose levels due to deficiency of insulin hormone secretion or when insulin resistance occurs, cells cannot effectively use the insulin produced²²⁻²⁴. It has long been known that glucose metabolism in serum in tubes filled with blood decreases over time. When the blood specimen has not been tested, the process of glycolysis can occur by the cellular components in it and can consume 5%–7% of the glucose contained in the sample every hour. The addition of fluoride as a glycolysis inhibitor can only be effectively used up to 4 hours of delay²³. Renal function tests are commonly used in clinical practice to look for kidney disease, the most common of which include serum urea, uric acid, and creatinine²⁵⁻²⁷. Uric acid (UA) an important role in renal function and GFR²⁸, being the end product of purine catabolism²⁹. Elevated UA levels are associated with the severity of hypertension, hyperuricemia, preeclampsia³⁰. Therefore, this study aims to compare the stability of the use of a gel vacutainer separator with a plain vacutainer.

MATERIALS AND METHODS

Research Design

The study design was experimental. The location of this research was carried out at the Clinical Pathology Laboratory Faculty of Health Sciences, Universitas Muhammadiyah Surabaya, Indonesia. The samples were taken randomly as many as 16 responden's did four treatments on each sample, P1: use of plain vacutainer for uric acid; P2: use of SST vacutainer for uric acid. Sample examination used serum; P3: plain vacutainer for glucose; P4: SST

vacutainer for glucose. Blood samples were taken as much as 3 ml using SST vacutainer and plain vacutainer. Preliminary tests were carried out by measuring the control serum 20 times and then making the Westgard rule.

Sample Preparation and Analysis

Sample criteria are not having a history of diabetes and gout, having a uric acid level of 4-7 mg/dl, and a glucose level of 80-110 mg/dl. The method of checking uric acid levels uses the Enzymatic Colorimetric method to determine uric acid through a reaction with uricas. H_2O_2 reacts under peroxidase catalysis with 3,5-dichloro-2-hydroxybenzene-sulfonic acid (DCHB) and 4-aminophenazone (PAP) to give purplish-red quinone imine dye as an indicator. While the method of checking glucose using GOD-PAP with the principle that glucose in the sample is oxidized to form gluconic acid and hydrogen peroxide. POD catalyzes hydrogen peroxide 4-Aminoatpyrene with phenol indicator to form quinone imine and water. Data analysis used a statistical test with paired t-test.

RESULTS

Uric Acid

Measurement of uric acid levels in SST vacutainer and plain vacutainer obtained the following results, the average uric acid levels using plain vacutainer and with SST vacutainer were 4.5875 mg/dl and 4.9250 mg/dl, respectively (Table 1). Data were analyzed using a paired t-test. There was a significant difference in uric acid levels between plain vacutainer and SST vacutainer ($p=0.000$).

Table 1. Comparison of serum uric acid using a plain vacutainer and with a SST vacutainer

	P1	P2
Mean	4.5875	4.9250
SD	0.56318	0.59048
Min	4.1	4.7
Max	6.0	6.5
Paired test	0.000	

P1 for plain vacutainer; P2 for SST vacutainer

Figure 1 shows the comparison of serum stability against uric acid. The mean uric acid levels using a plain vacutainer and with a SST vacutainer had consistent results in which the mean uric acid levels used SST vacutainer was higher than plain vacutainer.

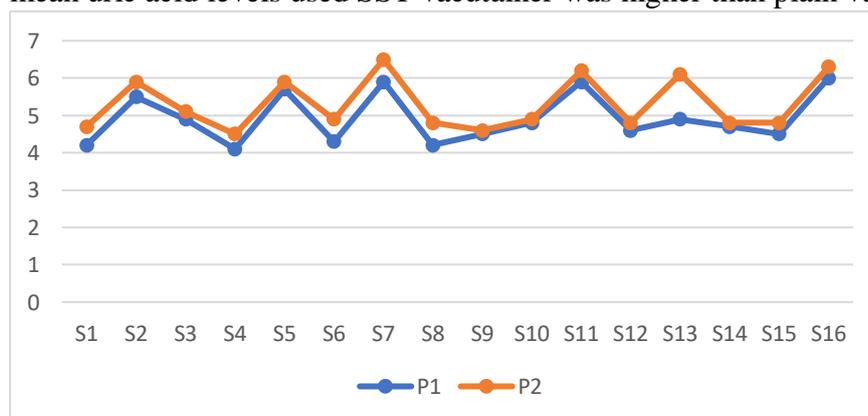


Figure 1. Comparison of serum stability against uric acid. P1 for plain vacutainer and P2 for SST vacutainer.

Glucose

Measurement of glucose levels in SST vacutainer and plain vacutainer obtained the

following results, the mean glucose levels using plain vacutainer and SST vacutainer were 90.64 mg/dl and 94.12 mg/dl (Table 2). Data were analyzed using paired t-test. There was a significant difference in glucose levels between plain vacutainer and SST vacutainer ($p = 0.000$).

Tabel 2. Comparison of serum glucose using a plain vacutainer and with a SST vacutainer

	P3	P4
Mean	90.64	94,12
SD	12.33	13,30
Min	85	87
Max	98	108
Paired test	0.00	

P3 for plain vacutainer; P4 for SST vacutainer

Figure 2 shows the comparison of serum stability against glucose. The mean glucose levels using a plain vacutainer and with a SST vacutainer had consistent results in which the mean glucose levels used SST vacutainer was higher than plain vacutainer.

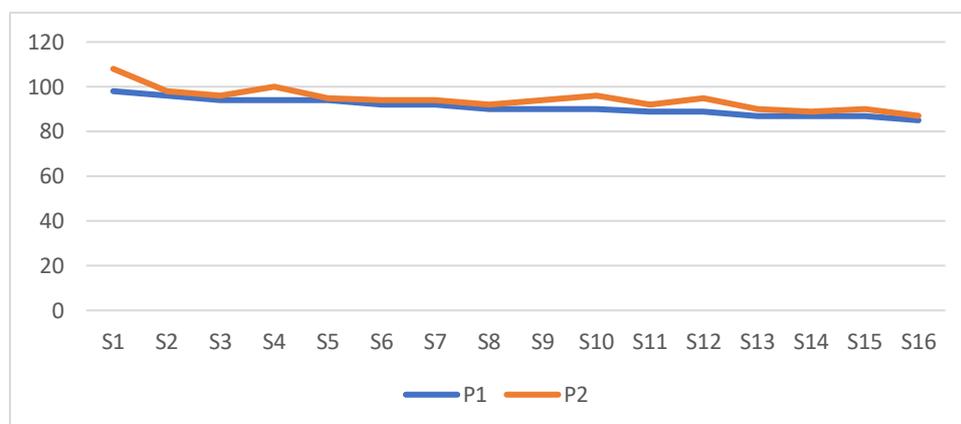


Figure 2. Comparison of serum stability against glucose. P1 for plain vacutainer and P2 for SST vacutainer.

The total processing time of the samples accommodated in the SST vacutainer was faster, with a mean of 24 minutes 51 seconds. At the same time, using a plain vacutainer blood collection tube takes a mean of 1 hour 3 minutes.

Tabel 3. Stability serum uric acid and glucose

	P1	P2	P3	P4
Mean	24':51"	1 hour:02"	24':49"	1hour:03"
Min	24':38"	59':50"	34':18"	59':58"
Max	35':38"	1 hour:05"	35':13"	1hour:06"

P1 for plain vacutainer, P2 for SST vacutainer for uric acid; P3 for plain vacutainer, P4 for SST vacutainer for glucose

DISCUSSION

This study showed that the mean values of plain vacutainer and SST vacutainer were within the normal range for uric acid and glucose levels. The mean uric acid level using SST vacutainer was higher than the mean uric acid level using plain vacutainer. These results also follow the study of urea levels conducted using three types of tubes, including serum separator tubes, lithium heparin vacutainers, and plasma separator tubes. Based on these results, the three tubes can be used as a substitute for serum for blood chemistry examination¹⁴. Glucose levels in this study had a higher average between SST vacutainer and plain vacutainer. This is influenced by the stability of glucose in serum to be used by cells other than blood cells, for

example by the presence of microbial contamination in serum²⁶.

Production and manufacture for SST tubes generally have a gel-specific gravity that varies relative to each factory, as Faught's research has shown that there are differences in the specific gravity of the separating gel used in some SST tubes and between tube lots²⁶. Although the SST vacutainer has the advantage of being able to optimize the workflow because of the composition of the silica clot activator and polymer gel which functions to separate serum from the clot, the results obtained are invalid or inaccurate, or inaccurate because the gel vacutainer separator also has a weakness. The gel should not be frozen because the physical composition of the gel can change so that there can be contamination between blood cells and serum, as well as instability and incompatibility of the analyte that does not match the patient sample³¹. In addition, many laboratories perform routine chemical analyzes with serum blood collection tubes containing a separating gel or polymer gel. However, previous studies have shown that gel tubes are not entirely perfect, although they have several advantages over ordinary tubes. The use of SST is generally disposable (disposable) so that it will increase the cost of purchasing the tube, especially for short-scale use at room temperature in the clinical laboratory²⁵.

While the advantages of SST vacutainer are workflow optimization short centrifugation time, sample processing and storage in the primary tube does not cause confusion for transfer to the secondary tube, produces better and more serum, can improve analyte stability, and reduce the rate of hemolysis during the separation process^{32,33}. A drawback of the SST vacutainer is the manufacturer's stated restrictions on sample handling for SST, which contains a gel that should not be frozen, as freezing and thawing can change the physical composition of the gel, resulting in contamination of blood cells and serum. Gel instability and analyte incompatibility are caused by flotation of gel separators that are not suitable for patient samples, physical instability of polymer-based polyesters under extreme temperature conditions, and the release of lubricants that can hinder the examination process¹⁴.

The total processing time of the samples accommodated in the SST vacutainer was faster than the plain vacutainer. The average sample processing time with a SST vacutainer is 25 minutes. At the same time, using an ordinary vacutainer blood collection tube takes an average of 1 hour 8 minutes¹⁷. The difference in time is because ordinary vacutainers require additional time for complete clotting on average for 35 minutes 50 seconds, while serum separator vacutainers only average about 4 minutes 38 seconds. This time calculation may differ if the work is carried out elsewhere with different room temperatures, tube sizes, and blood volumes. This is consistent with research showing that the use of gel is more profitable for laboratory technicians because it does not reduce Turn Around Time (TAT) and the presence of obstacles that can reduce sample transfer to secondary tubes and minimize the spread of potentially hazardous aerosols. Another advantage is that it can increase the stability of the analyte and reduce the rate of hemolysis during separation^{31,34,35}.

CONCLUSION

The uric acid and glucose level using a vacutainer separator gel was higher than the uric acid level using a plain vacutainer. The following types of vacutainer separator gel and plain vacutainer affected the quality of uric acid and glucose examination results.

ACKNOWLEDGMENTS

We would like to express our gratitude to the Head of Study Program, students and laboratory assistants of ClinicalPathology who have provided support and helped in this research.

CONFLICT OF INTEREST

The authors declare no conflict of interest.

REFERENCES

1. Saha D, Jain VK, Jain B, Tandey R. Good laboratory practice: design and utility. *Asian J Pharm Technol.* 2011;1(1):1–3. Available at: <https://ajptonline.com/AbstractView.aspx?PID=2011-1-1-1>
2. Hartono H, Subarniati R, Pudjirahardjo WJ, Judajana FM. Manajemen Pengetahuan untuk Keselamatan Pasien. *Indones J Clin Pathol Med Lab.* 2016;20(3):253–9.

- <http://dx.doi.org/10.24293/ijcpml.v20i3.474>
3. Hedayati M, Razavi SA, Boroomand S, Kheradmand Kia S. The impact of pre-analytical variations on biochemical analytes stability: A systematic review. *J Clin Lab Anal.* 2020;34(12):1–15. <https://doi.org/10.1002/jcla.23551>
 4. Kachhawa K, Kachhawa P, Varma M, Behera R, Agrawal D, Kumar S. Study of the Stability of Various Biochemical Analytes in Samples Stored at Different Predefined Storage Conditions at an Accredited Laboratory of India. *J Lab Physicians.* 2017;9(01):011–5. <https://doi.org/10.4103/0974-2727.187928>
 5. Putri AE, Indrasari YN, Hernaningsih Y. The effect of storage and time of blood specimen examination of plasma prothrombin time and activated partial thromboplastin time stabilities. *Indian J Forensic Med Toxicol.* 2020;14(3):1673–8. Available at: <https://repository.unair.ac.id/106358/>
 6. Muslim M, Suhariadi F, Damayanti NA, Purnomo W. The performance of medical laboratory technician based on situation awareness and psychological capital with the work engagement mediation. *Indian J Public Heal Res Dev.* 2018;9(1):199–202. Available at: <https://repository.unair.ac.id/92678/>
 7. Rahmanitarini A, Hernaningsih Y, Indrasari YN. The stability of sample storage for complete blood count (CBC) toward the blood cell morphology. *Bali Med J.* 2019;8:482. <https://doi.org/10.15562/bmj.v8i2.1369>
 8. Lestari A. Different Amount of Thrombocytes on Blood Storage for 24 Hours in Room and Refrigerator. *J Vocat Heal Stud.* 2019;3(2):59–62. <https://doi.org/10.20473/jvhs.V3.I2.2019.59-62>
 9. Kahar H. Keuntungan dan kerugian penjaminan mutu berdasarkan uji memastikan kecermatan (POCT). *Indones J Clin Pathol Med Lab.* 2018;13(1):38–41. <http://dx.doi.org/10.24293/ijcpml.v13i1.898>
 10. Cuhadar S, Koseoglu M, Atay A, Dirican A. The effect of storage time and freeze-thaw cycles on the stability of serum samples. *Biochem Medica.* 2013;23(1):70–7. <https://doi.org/10.11613/bm.2013.009>
 11. Bowen RAR, Remaley AT. Interferences from blood collection tube components on clinical chemistry assays. *Biochem Medica.* 2014;24(1):31–44. <https://doi.org/10.11613%2FBM.2014.006>
 12. Cuhadar S, Atay A, Koseoglu M, Dirican A, Hur A. Stability studies of common biochemical analytes in serum separator tubes with or without gel barrier subjected to various storage conditions. *Biochem Medica.* 2012;22(2):202–14. <https://doi.org/10.11613/bm.2012.023>
 13. Gómez Rioja R, Martínez Espartosa D, Segovia M, Ibarz M, Llopis MA, Bauça JM, et al. Laboratory sample stability. Is it possible to define a consensus stability function? An example of five blood magnitudes. *Clin Chem Lab Med.* 2018;56(11):1806–18. <https://doi.org/10.1515/cclm-2017-1189>
 14. Arslan FD, Karakoyun I, Basok BI, Aksit MZ, Baysoy A, Ozturk YK, et al. The local clinical validation of a new lithium heparin tube with a Barrier: BD vacutainer® barricor LH plasma tube. *Biochem Medica.* 2017;27(3):1–11. <https://doi.org/10.11613%2FBM.2017.030706>
 15. Lima-Oliveira G, Lippi G, Salvagno GL, Montagnana M, Picheth G, Guidi GC. Preanalytical management: Serum vacuum tubes validation for routine clinical chemistry. *Biochem Medica.* 2012;22(2):180–6. <https://doi.org/10.11613/bm.2012.021>
 16. Hegstad S, Spigset O, Helland A. Stability of 21 Antihypertensive Drugs in Serum Collected in Standard (Nongel) Serum Tubes Versus Tubes Containing a Gel Separator. *Ther Drug Monit.* 2020;42(2):335–40. <https://doi.org/10.1097/ftd.0000000000000708>
 17. Setiawan B, Nugraheni UR, Rahayu M. Vacutainer serum separator sebagai alternatif tabung penampung darah pada pemeriksaan kadar ureum. *J Muhammadiyah Med Lab Technol.* 2021;4(1):81. <http://dx.doi.org/10.30651/jmlt.v4i1.7447>
 18. Beeler MF. Medical Laboratory Technology. *Am J Trop Med Hyg.* 1963;12(5):835–835. <https://doi.org/10.4269/ajtmh.1963.12.835>
 19. Guder WG. History of the preanalytical phase: A personal view. *Biochem Medica.* 2014;24(1):25–30. <https://doi.org/10.11613%2FBM.2014.005>
 20. Bharath CL, Ramadurg B. Antidiabetic Activity of Phragmites karka (Retz.) in Alloxan

- Induced Diabetic Rats. *Res J Pharmacol Pharmacodyn.* 2013;5(6):371–5. Available at: <https://rjppd.org/AbstractView.aspx?PID=2013-5-6-21>
21. Abbas SH, Khedair SA. Study the Effect of Maternal Factors on Prevalence of Gestational Diabetes Mellitus and Effect of Treatment Types on Serum Blood Glucose. *Res J Pharm Technol.* 2021;14(10):5264–9. <http://dx.doi.org/10.52711/0974-360X.2021.00917>
 22. Hassan N, Shahwan M, Alkhoujah S, Jairoun A. Association between serum liver enzymes and metabolic syndrome among type 2 diabetes mellitus patients. *Age.* 2021;56(9.8):59–83. <https://doi.org/10.5958/0974-360X.2021.00188.8>
 23. Furqon A, Nurmukhlis H, Kasiman S. Stabilitas Konsentrasi Glukosa Darah Simpan Jangka Pendek Dalam Tabung Berteknologi Pemisah Jel. *Pharmaciana.* 2015;5(2):108–14. <http://dx.doi.org/10.12928/pharmaciana.v5i2.2310>
 24. Tandi J, Danthy R, Kuncoro H. Effect of Ethanol Extract from Purple Eggplant Skin (*Solanum melongena* L) On Blood Glucose Levels and Pancreatic B Cells Regeneration on White Rats Male Hypercholesterolemia-Diabetic. *Res J Pharm Technol.* 2019;12(6):2936–42. <https://doi.org/10.5958/0974-360X.2019.00494.3>
 25. Sirajwala HB, Sharma D, Agravatt AM. A study of serum total calcium and uric acid levels in preeclampsia Abstract: Is now with. *Indian J Basic Appl Med Res.* 2013;(1):50–6. Available at: <https://www.ijbamr.com/assets/images/issues/pdf/PDF%20DECEMBER%2013%20%2050-56.pdf.pdf>
 26. Faught RC, Marshall J, Bornhorst J. Solution densities and estimated total protein contents associated with inappropriate flotation of separator gel in different blood collection tubes. *Arch Pathol Lab Med.* 2011;135(9):1081–4. <https://doi.org/10.5858/2010-0488-oar.1>
 27. Murtadha JH, Razzaq HA. Association of serum renal function levels with heart failure disease in iraqi patients. *Res J Pharm Technol.* 2021;14(5):2464–6. <https://doi.org/10.5958/0974-360X.2019.00494.3>
 28. Dhivya S, Gangopadhyay S, Kumar P, Sarkar G. Serum creatinine and eGFR are affected in female hypothyroid patients with poor Thyroid control. *Asian J Pharm Technol.* 2020;10(4). <http://dx.doi.org/10.5958/2231-5713.2020.00040.9>
 29. Mohammed OJ, Saeed AM, Mohammed IS. RP–HPLC Developed Method for Uric Acid Estimation in Human Serum. *Res J Pharm Technol.* 2019;12(10):4703–8. <https://doi.org/10.5958/0974-360X.2019.00810.2>
 30. Nisa U, Astana PRW, Kuncoro H. The effect of Antihypertensive Herb formula of Indonesian traditional medicines against serum uric acid levels in mild Hypertensive patients. *Res J Pharm Technol.* 2021;14(1):254–8. <http://dx.doi.org/10.5958/2231-5713.2020.00040.9>
 31. Kocijancic M, Cargonja J, Delic-Knezevic A. Evaluation of the BD Vacutainer® RST blood collection tube for routine chemistry analytes: Clinical significance of differences and stability study. *Biochem Medica.* 2014;24(3):368–75. <https://doi.org/10.11613/bm.2014.039>
 32. Martsiningsi, Otnel. Gambaran Kadar Asam Urat Darah Metode Basah (Uricase-PAP) Pada Sampel Serum dan Plasma. *J Teknol Lab.* 2016;5(1):20–6. Available at: <https://www.teknolabjournal.com/index.php/Jtl/article/view/72/51>
 33. Kösem A, Topçuoğlu C, Sezer S, Turhan T, Cevher ŞK, Yenigün EC, et al. Comparison of some biochemical tests in different blood collection tubes in hemodialysis patients. *Turkish J Biochem.* 2020;45(1):26–36. <http://dx.doi.org/10.1515/tjb-2018-0341>
 34. Erdal EP, Mitra D, Khangulov VS, Church S, Plokhoy E. The economic impact of poor sample quality in clinical chemistry laboratories: results from a global survey. *Ann Clin Biochem.* 2017;54(2):230–9. <https://doi.org/10.1177/0004563216651647>
 35. Nwe WWP, Thwin AMM, San Yi M, Yee KT, Oo MS, Rahman NIBA, et al. Serum Uric Acid, Lipid Profile and Atherogenic Index of Plasma in Dipper and Non-dipper Normotensive Subjects. *Res J Pharm Technol.* 2021;14(5):2511–6. <https://doi.org/10.52711/0974-360X.2021.00442>